



Quick-Check Mitt

Single Patient Use Only

Rx Only



IMPORTANT INFORMATION

Please read all instructions, warnings, and precautions before use. Correct application is essential for proper functioning of product. A physician or other licensed independent practitioner, primarily responsible for the patient's ongoing care, orders this product in accordance with hospital policy and law and regulation. Follow the instructions of your physician (or other licensed independent practitioner) for length and duration of use. Inform the patient, patient's family and/or legal guardian about the intended use, warnings and precautions of this device.

INTENDED USE

Hand control mittens are intended for mildly agitated patients who disrupt medical treatment and/or cause harm to themselves and/or others. Hand control mittens control hand and finger movements and/or limits limb movements.

WARNINGS

- Incorrect use of this product can result in injury or death.
- Do not use this device without authorization by a physician or other licensed independent practitioner.
- Do not secure straps to bed side rails.
- Do not expose this product to any source of flame. Materials in this device are susceptible to ignition or burning.



PRECAUTIONS

Ensure that the product does not restrict circulation or result in discomfort. Monitor the patient frequently, in accordance with hospital policy and law and regulation. Inspect hospital equipment that is used in conjunction with this product. Check hospital equipment for any moving parts that may interfere with proper function of the product. If the product is attached to hospital equipment, be sure to attach the product to a location that moves with the patient. If the product is on the patient while in bed, make sure that bed side rails are up. Secure any excess materials away from the patient's reach and to help prevent tripping and/or falling. In the event of an emergency, the product can be cut off the patient.

INSTRUCTIONS FOR USE

Quick-Check Mitt

1. Slide the patient's hand into the mitten with the palm facing down. The inspection flap should rest on top of the hand.
2. Secure wrist closure by feeding the hook and loop strap through the plastic buckle and back onto itself.
3. To view patient's hand/fingers, reach under the inspection flap and detach the hook and loop



Quick-Check Mitt

Single Patient Use Only

Rx Only



IMPORTANT INFORMATION

Please read all instructions, warnings, and precautions before use. Correct application is essential for proper functioning of product. A physician or other licensed independent practitioner, primarily responsible for the patient's ongoing care, orders this product in accordance with hospital policy and law and regulation. Follow the instructions of your physician (or other licensed independent practitioner) for length and duration of use. Inform the patient, patient's family and/or legal guardian about the intended use, warnings and precautions of this device.

INTENDED USE

Hand control mittens are intended for mildly agitated patients who disrupt medical treatment and/or cause harm to themselves and/or others. Hand control mittens control hand and finger movements and/or limits limb movements.

WARNINGS

- Incorrect use of this product can result in injury or death.
- Do not use this device without authorization by a physician or other licensed independent practitioner.
- Do not secure straps to bed side rails.
- Do not expose this product to any source of flame. Materials in this device are susceptible to ignition or burning.



PRECAUTIONS

Ensure that the product does not restrict circulation or result in discomfort. Monitor the patient frequently, in accordance with hospital policy and law and regulation. Inspect hospital equipment that is used in conjunction with this product. Check hospital equipment for any moving parts that may interfere with proper function of the product. If the product is attached to hospital equipment, be sure to attach the product to a location that moves with the patient. If the product is on the patient while in bed, make sure that bed side rails are up. Secure any excess materials away from the patient's reach and to help prevent tripping and/or falling. In the event of an emergency, the product can be cut off the patient.

INSTRUCTIONS FOR USE

Quick-Check Mitt


1. Slide the patient's hand into the mitten with the palm facing down. The inspection flap should rest on top of the hand.
2. Secure wrist closure by feeding the hook and loop strap through the plastic buckle and back onto itself.
3. To view patient's hand/fingers, reach under the inspection flap and detach the hook and loop








closure. Pull the flap back to expose the hand.

4. To close the inspection flap, tuck the flap over the end of the mitten and secure the hook and loop closure. **NOTE: This mitten is not designed with an optional bed attachment strap.**




Quick-Check Mitt with Buckle

1. Follow the instructions for use for the Quick Check Mitt. Next, take the end of the excess strap from the hook and loop closure and thread it through the seawave buckle.
2. This mitten is designed to be used with an optional bed attachment strap. To apply the bed attachment strap, take the end of the strap and feed it through the loop located near the



bottom of the mitten near the sew-in label.

3. Thread the end of the strap through the seawave buckle and pull the entire length of the strap through the buckle.
4. Attach the end of the strap to the portion of the bed frame that moves with the patient using quick-release ties. Please follow the instructions for quick-release ties provided below.



CARE INSTRUCTIONS

This product is disposable and should not be laundered or reused. DISCARD AFTER USE.





Improving Care. Improving Business.

Distributed by DeRoyal
200 DeBusk Lane
Powell, TN 37849 U.S.A.
888.938.7828 • 865.938.7828

©2010 DeRoyal. All Rights Reserved.
Part #0-1813 Revised 7/10


QUICK-RELEASE TIES

Attach the strap(s) using quick-release ties by following the step-by-step instructions below.

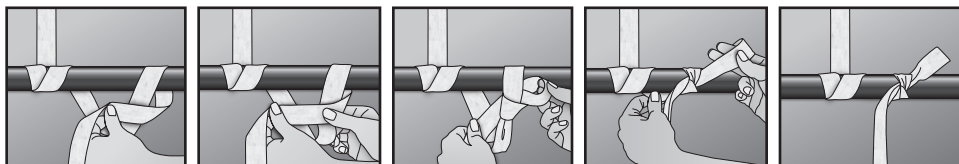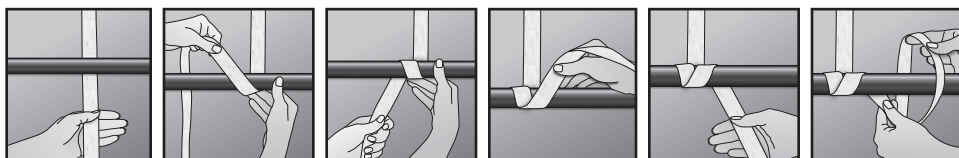




closure. Pull the flap back to expose the hand.

4. To close the inspection flap, tuck the flap over the end of the mitten and secure the hook and loop closure. **NOTE: This mitten is not designed with an optional bed attachment strap.**




Quick-Check Mitt with Buckle

1. Follow the instructions for use for the Quick Check Mitt. Next, take the end of the excess strap from the hook and loop closure and thread it through the seawave buckle.
2. This mitten is designed to be used with an optional bed attachment strap. To apply the bed attachment strap, take the end of the strap and feed it through the loop located near the



bottom of the mitten near the sew-in label.

3. Thread the end of the strap through the seawave buckle and pull the entire length of the strap through the buckle.
4. Attach the end of the strap to the portion of the bed frame that moves with the patient using quick-release ties. Please follow the instructions for quick-release ties provided below.



CARE INSTRUCTIONS

This product is disposable and should not be laundered or reused. DISCARD AFTER USE.



Improving Care. Improving Business.

Distributed by DeRoyal
200 DeBusk Lane
Powell, TN 37849 U.S.A.
888.938.7828 • 865.938.7828

©2010 DeRoyal. All Rights Reserved.
Part #0-1813 Revised 7/10

QUICK-RELEASE TIES

Attach the strap(s) using quick-release ties by following the step-by-step instructions below.

