


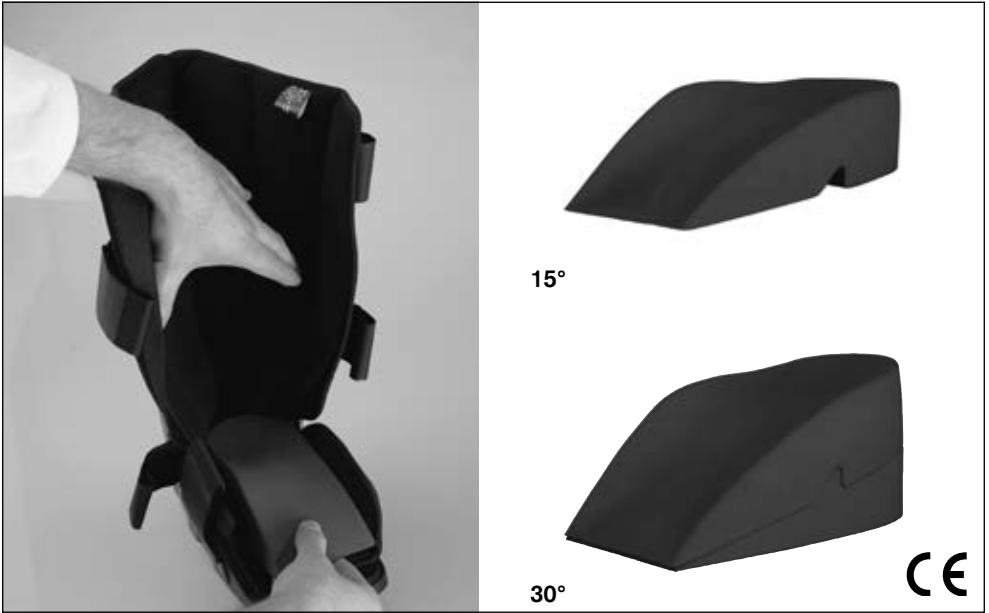

29S35

DE Gebrauchsanweisung

EN Instructions for use

INFORMATION

Datum der letzten Aktualisierung: 2014-12-05

- Lesen Sie dieses Dokument aufmerksam durch.
- Beachten Sie die Gebrauchsanweisung 647G978 (Malleo Immobil Walker).
- Beachten Sie die Gebrauchsanweisung 647G1119 (Infinity Air Walker).
- Beachten Sie die Gebrauchsanweisung 647G1122 (Infinity Double Air Walker).

Fersenkeile zur Einlage in Malleo Immobil Walker high 50S10-1, Malleo Immobil Air Walker high 50S12-1, Malleo Immobil Achilles Walker 50S17, Infinity Air Walker high 50S19 und Infinity Double Air Walker high 50S24.



Feucht abwischbar

Artikelnummer	Seite	Schuhgröße
29S35=L-S/M	Links	31 – 42
29S35=R-S/M	Rechts	31 – 42
29S35=L-L/XL	Links	43 – 50
29S35=R-L/XL	Rechts	43 – 50

English

INFORMATION

Date of the last update: 2014-12-05

- Please read this document carefully.
- Follow the instructions for use 647G978 (Malleo Immobil Walker).
- Follow the instructions for use 647G1119 (Infinity Air Walker).
- Follow the instructions for use 647G1122 (Infinity Double Air Walker).

Heel wedges for use as an insole in Malleo Immobil Walker high 50S10-1, Malleo Immobil Air Walker high 50S12-1, Malleo Immobil Achilles Walker 50S17, Infinity Air Walker high 50S19 und Infinity Double Air Walker high 50S24.



Damp wipeable

Article number	Side	Shoe size
29S35=L-S/M	Left	31 – 42
29S35=R-S/M	Right	31 – 42
29S35=L-L/XL	Left	43 – 50
29S35=R-L/XL	Right	43 – 50



Otto Bock HealthCare GmbH
 Max-Näder-Straße 15 · 37115 Duderstadt/Germany
 T +49 5527 848-0 · F +49 5527 72330
 healthcare@ottobock.de · www.ottobock.com

Ottobock has a certified Quality Management System in accordance with ISO 13485.