




STEP 1: Bench Adjustment

Adjust Shank Alignment to 0°. Adjust Plantarflexion Range of Motion to 0°. Adjust Dorsiflexion Range of Motion to 0°.

STEP 2: Static Alignment


Adjust Shank Alignment. Note: Plantarflexion and Dorsiflexion ROM = 0°

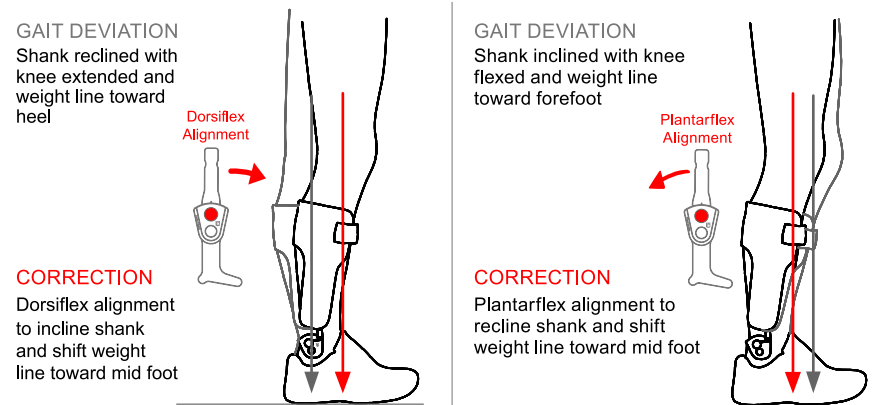

QUIET STANDING

STEP 3: Swing Phase Alignment

Adjust Ankle Alignment. Note: Plantarflexion and Dorsiflexion ROM = 0°

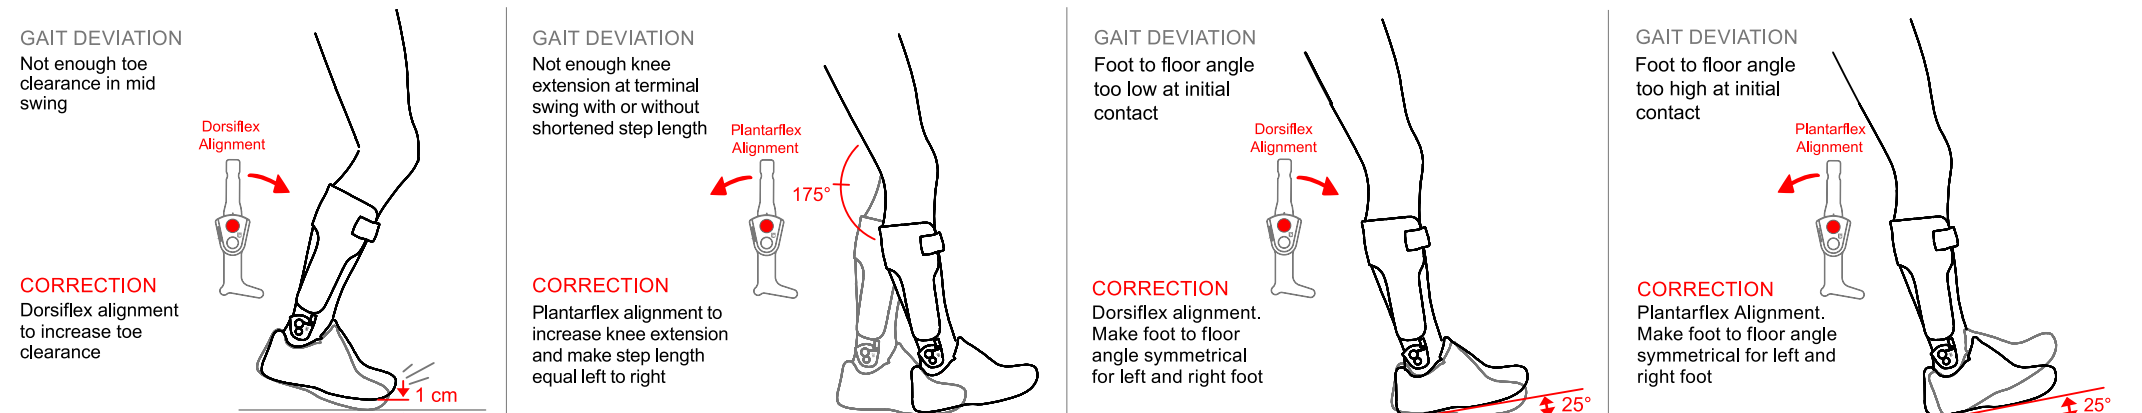


MID SWING

TERMINAL SWING

INITIAL CONTACT

STEP 4A: Early Stance Phase Adjustment


Adjust Plantarflexion ROM. If foot to floor angle at initial contact decreases with increased PF ROM, return the previous ROM setting or increase spring stiffness. Note: DF ROM = 0°

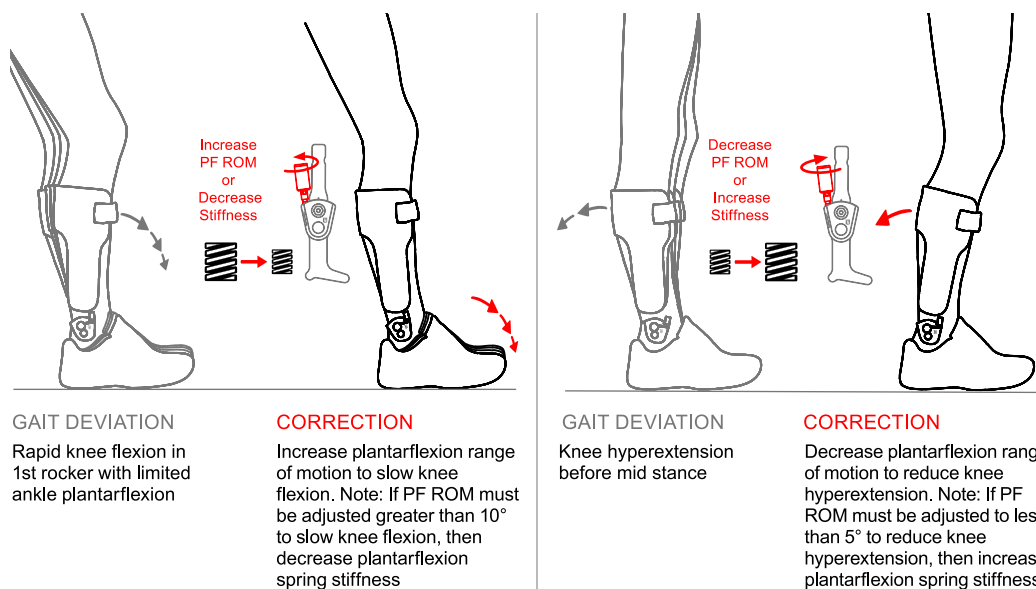

1ST ROCKER

STEP 4B: Late Stance Phase Adjustment

Adjust Dorsiflexion ROM.

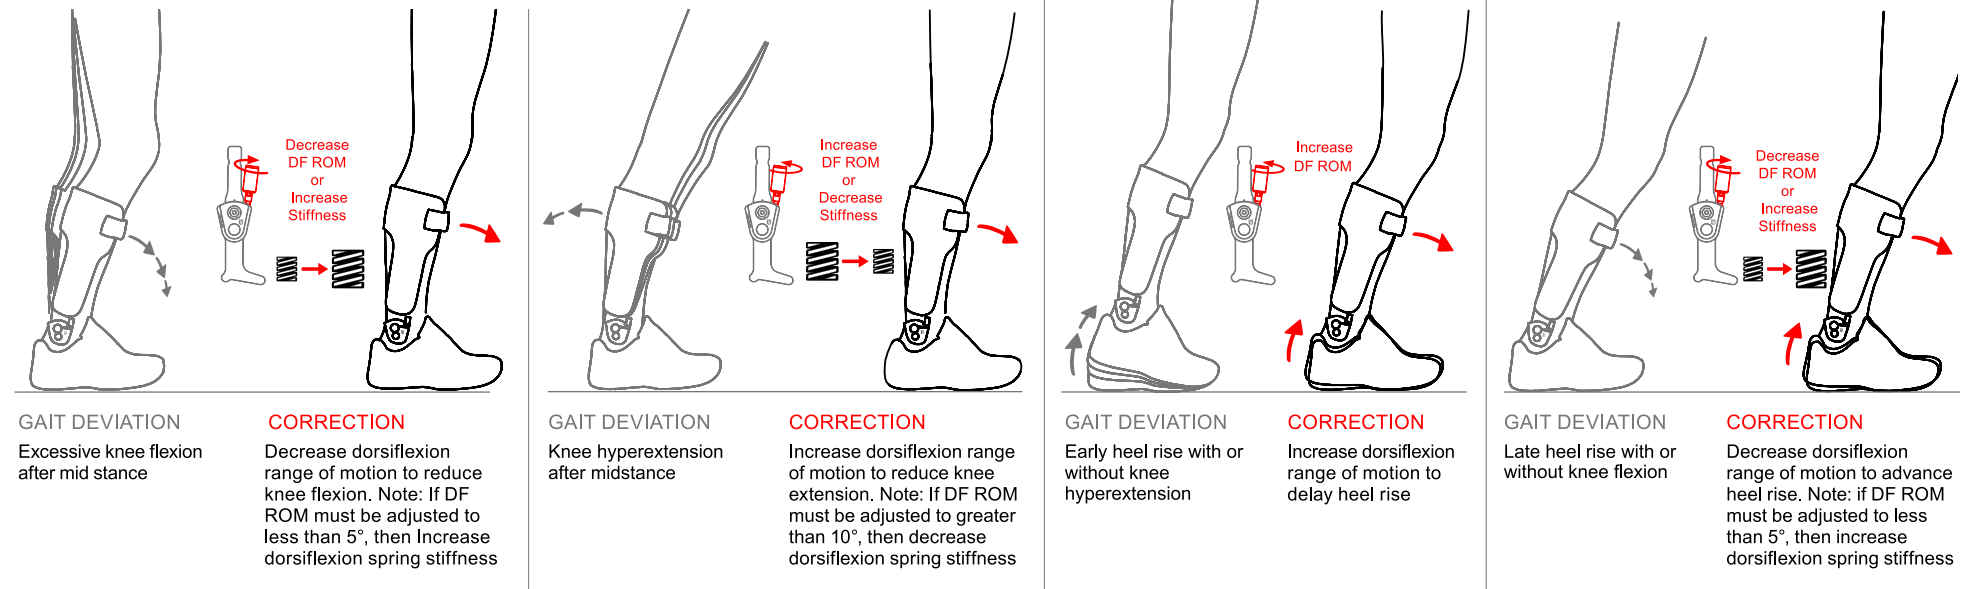

2ND ROCKER

3RD ROCKER