


FDE SPRING CATEGORY (FIRMNESS) SELECTION

Most Common Starting Point

Category number three **3** spring is a good starting point. From here the AFO can be tuned Firmer or Softer based on the patient needs. The simple four-bolt system makes changing the spring quick and easy

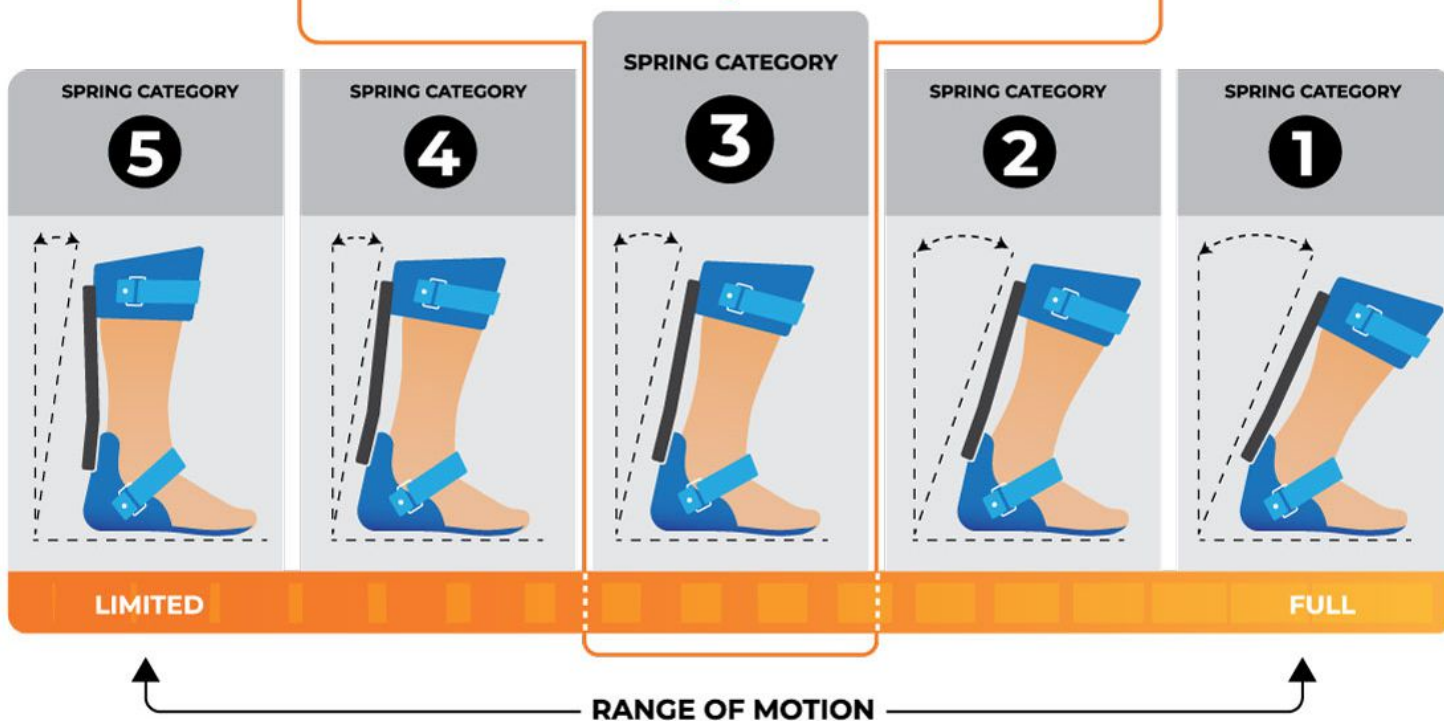

Because every patient has unique needs there are no specific weight limitations that aid in spring choice. Choose the category based on your patient assessment.